

ETF¹²⁸/Mx Ascending Timed Vibration Test (TVT) Results *


Patient: _____

Date: _____

Right Hallux

Neuropathy Risk


- High
- Moderate
- Low

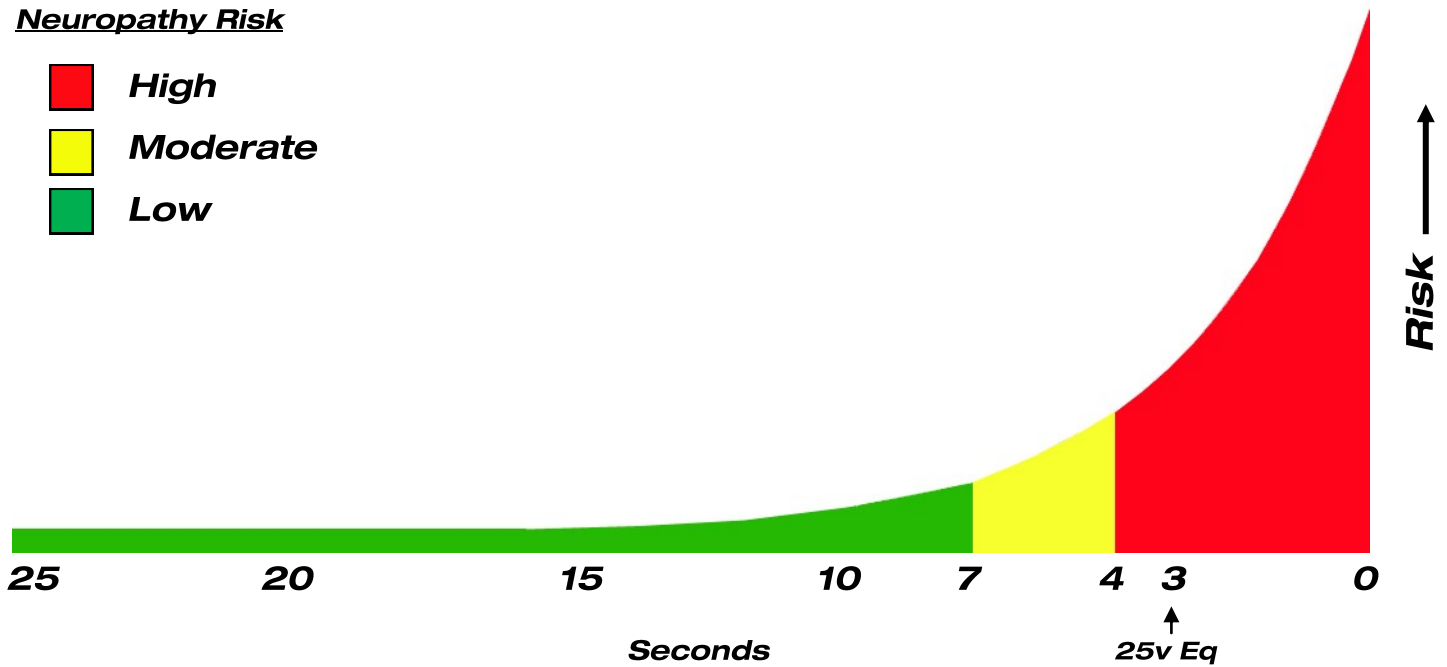

Left Hallux

Neuropathy Risk

- High
- Moderate
- Low

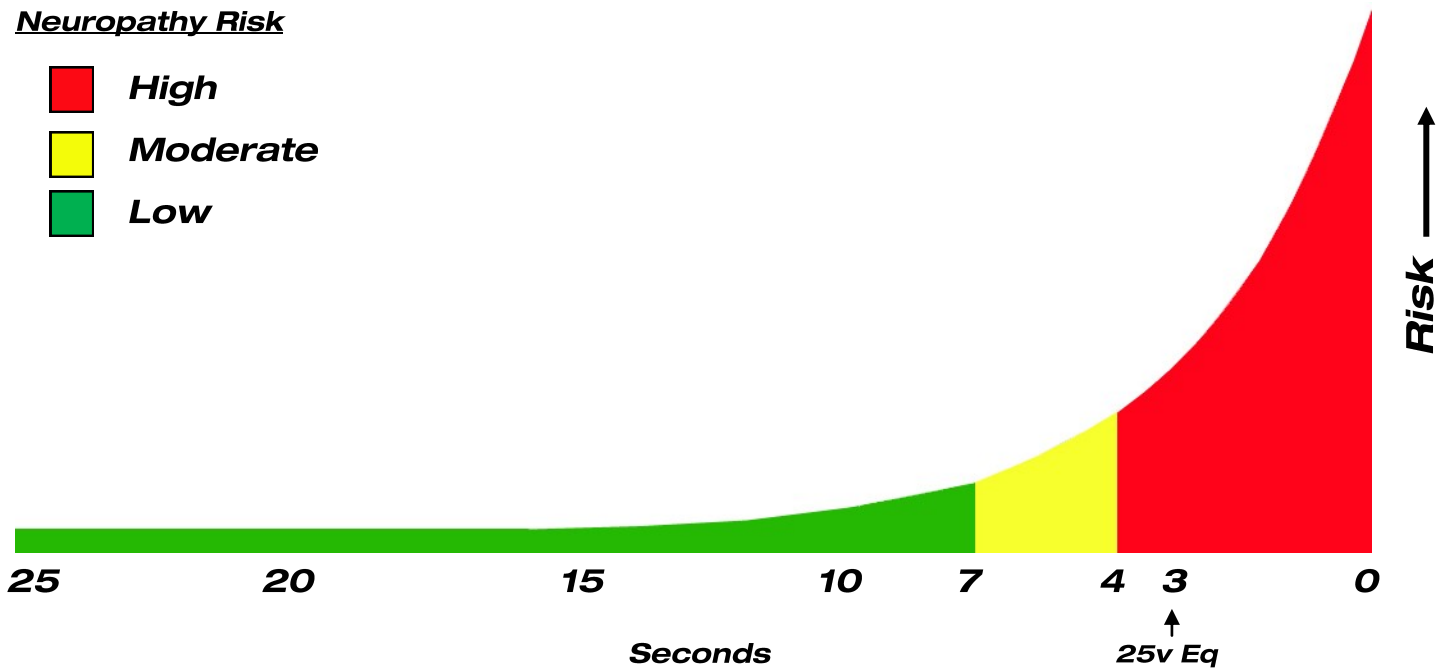

* Based on testing at the dorsal aspect of the distal phalanx of the hallux in 128Hz Descending Mode. Results reflect status of vibratory sensation which gauges large fiber nerve function. Neuropathy scale is based on results cited in O'Brien and Karem, J Am Podiatr Med Assoc. 2014 Mar;104(2):134-40. doi: 10.7547/0003-0538-104.2.134.